

# Real-Time Ultrasonic Assessment of Progressive Proteoglycan Depletion in Articular Cartilage

Q Wang<sup>1</sup>, YP Zheng<sup>1</sup>, L Qin<sup>2</sup>, QH Huang<sup>1</sup>, WL Lam<sup>3</sup>, G Leung<sup>1</sup>, X Guo<sup>3</sup>, HB Lu<sup>2</sup>

1. Department of Health Technology and Informatics, The Hong Kong Polytechnic  
University, Hong Kong, China

2. Musculoskeletal Research Laboratory, Department of Orthopaedics and Traumatology,  
The Chinese University of Hong Kong, Hong Kong, China

3. Department of Rehabilitation Sciences, The Hong Kong Polytechnic University, Hong  
Kong, China

Running Title: **Ultrasonic Monitoring of Proteoglycan Depletion**

\* Correspondence address:

Dr. Zheng Yongping

Department of Health Technology and Informatics

The Hong Kong Polytechnic University

Kowloon

Hong Kong SAR, China

Tel: 852-27667664

E-mail: ypzheng@iee.org

## Abstract

The loss of proteoglycan (PG) is regarded as one of the early signs of osteoarthritis (OA), thus observing the progress of PG loss would be useful for the early detection of OA. In this study, high-frequency ultrasound was used to monitor and analyze the trypsin-induced progressive degeneration in articular cartilage. Full-thickness cartilage-bone specimens ( $n = 10$ ) prepared from normal bovine patellae were digested using 0.25% trypsin solution for different periods of time to evaluate the dynamic of the digestion process. The trypsin penetration front was observed in M-mode image, which was acquired using a nominal 50 MHz focused transducer. The transient speed of the digestion process was estimated from the image. The digestion fraction, which represents the ratio of the digestion depth to the total cartilage thickness, was estimated from ultrasound data and histology sections. With ultrasound, the digestion fraction observed in the 10 specimens ranged from 64 to 99%, and was correlated to that measured by histology ( $R^2 \geq 0.63$ ,  $p < 0.05$ ). It was found that the digestion speed decreased nonlinearly with depth from  $0.61 \pm 0.16 \mu\text{m/s}$  (mean  $\pm$  SD) in the superficial zone to  $0.04 \pm 0.02 \mu\text{m/s}$  in a region located at 70% of the cartilage thickness in depth. The relationship between the digestion depth and the exposure duration in trypsin could be described using a 3<sup>rd</sup> order polynomial function. The full-thickness of digested and undigested tissues was also measured using caliper, estimated from ultrasound data and histology sections, and compared. These findings indicate that ultrasound could provide useful information about the trypsin-induced progressive PG depletion in articular cartilage. Therefore, ultrasound represents a useful tool to evaluate the dynamic of models of OA *in vitro* in cartilage specimens in a research environment, and this would ultimately help the *in-vitro* examination of articular cartilage for research related to model of OA from the early stages of tissue degradation.

**Keywords:** Articular cartilage; Ultrasound; Proteoglycan depletion; Trypsin digestion; Osteoarthritis

# 1 INTRODUCTION

2 Articular cartilage is a low frictional, load-bearing soft tissue, which covers the  
3 articulating bony ends in diarthrodial joints. This tissue is a multi-phasic hydrated  
4 mixture mainly composed of 5–10% proteoglycan (PG), 10–20% collagen, and 60–80%  
5 water (Mow et al. 2005). It has been discovered that the aggregating PGs are bio-  
6 macromolecules negatively charged and enmeshed in the collagen matrix (Lai et al. 1991;  
7 Maroudas 1976). PGs are also involved in binding cations and water. Therefore, they  
8 play an important role in electrochemical mechanical properties of articular cartilage such  
9 as shear modulus (Zhu et al. 1993), compressive modulus (Qin et al. 2002; Zheng et al.  
10 2001), swelling strain (Narmoneva et al. 1999; Wang and Zheng 2006) and swelling  
11 aggregate modulus (Flahiff et al. 2004; Narmoneva et al. 2002; Wang et al. 2007).

12

13 Osteoarthritis (OA) is considered as one of the most common joint diseases, which in its  
14 advanced stage is characterized by a partial or total loss of the cartilage tissue and the  
15 exposition of the bone across the joint. At a late stage, swelling and pain can lead to the  
16 loss of the joint functions, and consequently immobility. It was suggested that a  
17 macromolecular degradation happens at the early- and mid-stages of the cartilage  
18 degeneration and is catalyzed by proteolytic enzymes (Sandy 2003). The increase of  
19 tissue hydration, loss of PGs, and damage of collagen fibrils were regarded as the earliest  
20 signs of cartilage degeneration during OA (Armstrong and Mow 1982; Martini 2004;  
21 Sandy 2003; Torzilli et al. 1990). Since these early signs are not easy to detect, generally,  
22 articular cartilage has already suffered serious and irreversible damage when OA can be  
23 clinically diagnosed using X-ray. Therefore, detecting early signs of cartilage

1 degeneration, such as the loss of PGs, would allow an early diagnosis of the disease, and  
2 a timely treatment.

3  
4 During the past decades, several methods and techniques have been developed and used  
5 for the evaluation of the cartilage degeneration. Histological assays are traditionally used  
6 for the assessment of cartilage degeneration by binding different stains, such as safranin  
7 O, toluidine blue, haematoxylin and eosin (H&E), and alcian blue, to different  
8 compositions (Lyons et al. 2006). However, this method is time-consuming and invasive  
9 since it requires removing samples from the tissue using biopsy. Imaging techniques,  
10 such as magnetic resonance imaging (MRI) (Batiste et al. 2004; Raynauld et al. 2006)  
11 and ultrasonography (Yang et al. 2005), have recently been used in clinical practice  
12 providing non-invasive approaches to measure morphological damages in articular  
13 cartilage. The damages include irregularities at the cartilage-bone interface and the loss  
14 of the cartilage volume. High frequency ultrasound characterization of articular cartilage  
15 has been the subject of many recent investigations. These studies have reported on the  
16 suitability of ultrasound for the measurement of articular cartilage thickness (Adam et al.  
17 1998; Joiner et al. 2001; Jurvelin et al. 1995; Laasanen et al. 2002; Lefebvre et al. 1998;  
18 Myers et al. 1995; Toyras et al. 2001; Yao and Seedhom 1999). Various acoustic  
19 parameters including the speed of sound (Agemura et al. 1990; Myers et al. 1995),  
20 attenuation (Senzig et al. 1992; Toyras et al. 1999), echo pattern (Kim et al. 1995; Myers  
21 et al. 1995; Saied et al. 1997), and reflection and scattering coefficients (Adler et al. 1992;  
22 Cherin et al. 1998, 2001; Hattori et al. 2003, 2005; Laasanen et al. 2002; Nieminen et al.  
23 2002; Pellaumail et al. 2002; Toyras et al. 1999) have been used for the characterization

1 of articular cartilage in healthy and osteoarthritic conditions. 3D ultrasound measurement  
2 of articular cartilage has also been reported (Lefebvre et al. 1998). A miniaturized A-  
3 mode ultrasound probe has been developed for arthroscopic use (Hattori et al. 2005;  
4 Laasanen et al. 2002). In addition, ultrasound has been combined with indentation and  
5 compression for the measurement of tissue elasticity (Fortin et al. 2003; Laasanen et al.  
6 2002; Saarakkala et al. 2003; Toyras et al. 1999; Zheng and Mak 1996; Zheng et al. 2001,  
7 2002, 2004a, 2005). However, experiments reported in most of these previous studies  
8 were performed *in vitro* and acoustic and mechanical properties were measured at only  
9 two time points, before and after cartilage degeneration.

10  
11 Recently, the dynamic of trypsin penetration during digestion into the cartilage has been  
12 investigated using ultrasound (Nieminen et al. 2002; Zheng et al. 2004b). In the early  
13 stage of OA, PGs are continuously being broken down and PG fragments are released  
14 from the matrix leading to the net loss of PGs. Similarly, trypsin digestion can induce a  
15 similar cleavage of PG aggregates. Therefore digestion of cartilage using this agent has  
16 been widely used as a model of OA. Traditionally, the effects of trypsin in cartilage have  
17 been evaluated by histology at discrete time points only. Since variations in the cartilage  
18 thickness and in the distributions of PGs and chondrocytes are commonly observed  
19 between different specimens (Moody et al. 2006), it is difficult to control the digestion  
20 process by trypsin using histological techniques. On the other hand, it has been well  
21 documented that the loss of PGs causes a significant reduction of the tissue elasticity,  
22 which is directly related to the acoustic impedance. It has been shown that a rupture of  
23 impedance between digested and undigested tissue leads to the detection of an ultrasound

1 echo at the interface between these tissues. The motion of this echo toward the bone, as  
2 trypsin penetrates deeper in the cartilage, has been observed in M-mode images  
3 (Nieminen et al. 2002; Zheng et al. 2004b).

4  
5 In this study, we investigate this ultrasound approach for tracking in real-time the  
6 penetration of trypsin and measuring the transient speed of digestion. To validate this  
7 method, measurements performed with ultrasound are compared with those obtained  
8 using histology. Our results might provide useful information about the dynamic of the  
9 digestion by trypsin and therefore some insight on the early stages of OA. They might  
10 also provide a validation of the ultrasound approach for a real time evaluation of models  
11 of OA.

## 13 MATERIALS AND METHODS

### 14 *Specimen preparation*

15 Fresh mature bovine patellae ( $n = 10$ ) without apparent lesions were obtained from a  
16 local butcher shop within 6 hours of slaughter and stored at  $-20^{\circ}\text{C}$  until further  
17 preparation. One cartilage-bone plug was obtained from the upper-medial area of each  
18 patella using a metallic punch with a diameter of 6.35 mm (Wang and Zheng 2006). The  
19 cartilage-bone plugs were wrapped in wet gauze soaked with physiological saline and  
20 stored at  $-20^{\circ}\text{C}$  until ultrasound examination. Before examination, each plug was cut into  
21 two parts ( $1/3$  and  $2/3$ ) (Fig. 1a). The  $2/3$  portion samples were exposed to trypsin  
22 digestion and monitored by ultrasound simultaneously. Both trypsin-treated ( $2/3$  portion)  
23 and control ( $1/3$  portion) samples were assessed using histology.

1

2 *Ultrasound examination and signal processing*

3 Before ultrasound examination, each sample was first thawed for three hours in  
4 physiological saline solution (0.15 M NaCl) at room temperature ( $21\pm1^{\circ}\text{C}$ ). Then, the  
5 sample was fixed using the rubber gel (Blu-Tack, Thomastown, Australia) to the bottom  
6 of the container. The outer ring of the surface of the cartilage disc, approximately 0.6 mm  
7 in thickness, was gently covered by the rubber gel to ensure a trypsin penetration into the  
8 cartilage sample from the surface top layer toward the cartilage-bone interface (Fig. 1).  
9 The sample was then submerged in 0.15 M saline solution for another one hour. Then, the  
10 saline solution was rapidly removed from the container using an injection syringe and  
11 replaced with a trypsin solution (0.25%, Cat. No. 25200-056, Gibco, Invitrogen Inc.,  
12 Burlington, ON, Canada). The fluid replacement was performed in approximately 30 s.

13

14 Trypsin digestion in the sample was monitored using an ultrasound measurement system  
15 developed in our laboratory (Fig. 1b) (Wang and Zheng 2006). An ultrasound  
16 pulser/receiver (Model 5601A, Panametrics, Waltham, MA, USA) was used to drive a  
17 nominal 50 MHz focused ultrasound transducer (Model PI50-2, Panametrics, Waltham,  
18 MA, USA). This transducer had a focal length of 12.7 mm, a diameter of 6.35 mm, a -  
19 6dB beamwidth of 0.1 mm and a -6dB focal zone depth of 0.95 mm. The focal zone of  
20 the transducer was positioned in the centre of the sample using a 3D translating stage  
21 (Model R301MMX/2201MMXY, Ball Slide Positioning Stages, Del-Tron Precision Inc.,  
22 Bethel, CT, USA). Ultrasound echoes reflected or backscattered from internal structures  
23 in the cartilage sample were collected by the transducer, amplified by the receiver, and

1 digitized by an 8-bit A/D converter at a sampling rate of 500 MHz (CompuScope  
2 8500PCI, Gage, ON, Canada). Digitized signals were displayed on the computer monitor  
3 in real-time and simultaneously saved on the hard drive for offline data analysis. A  
4 custom-designed software developed in our laboratory for the ultrasound measurement of  
5 motion and elasticity (Zheng et al. 2001, 2004b) was used to control data collection and  
6 display.

7

8 During the progressive digestion of cartilage by trypsin, M-mode data were collected at a  
9 pulse repetition frequency (PRF) of 0.6 Hz. M-mode images are particularly suitable for  
10 monitoring of movements of tissue interfaces, and have been commonly used to study the  
11 motion of heart walls. Experiments were carried out at room temperature ( $21\pm1^{\circ}\text{C}$ ). As  
12 the trypsin penetrated into the cartilage tissue and broke down PG aggregates, an echo  
13 appeared at the interface between digested and undigested tissues. With time, this echo  
14 was detected deeper in the tissue, and gave rise to the inclined trace observed in M-mode  
15 images (Fig. 2). Markers were manually positioned along the trace in the M-mode images  
16 at different depths corresponding to the location of the digestion front at different time  
17 points. From the locations of these markers, our software automatically generated by  
18 interpolation the curve representing the depth of this front as a function of time. The  
19 positioning of the markers was repeated six times for each specimen to obtain six  
20 different interpolation curves, which were averaged together. From this averaged curve,  
21 were extracted both the transient speed of trypsin penetration and the digestion fraction.  
22 The digestion fraction was defined as the ratio of the digestion depth to the total cartilage  
23 thickness. For the comparison between some ultrasonic and histological measurements,



1 the digestion fraction was preferred to the absolute digestion depth, because it is not  
2 affected by variations of the ultrasound speed between samples or a potential shrinkage  
3 induced by the histological process.

4  
5 In this study, the full thickness of the cartilage layer ( $h$ ) was calculated by the following  
6 equation.

$$h = c_{AC} \times T_{AC} / 2$$

7  
8 where  $T_{AC}$  is the time of flight that the ultrasound echoes travel through the cartilage  
9 tissue. The ultrasound speed in articular cartilage  $c_{AC}$  was calculated using a non-contact  
10 ultrasonic method (Patil et al. 2004). The average sound speed in the full-thickness  
11 cartilage layer soaked in 0.15 M saline was 1675 m/s for the normal specimens. Since the  
12 echoes reflected from the cartilage-bone interface shifted slightly during the digestion  
13 (Fig. 2), indicating that the trypsin digestion generated a corresponding slight change in  
14 the ultrasound speed in the tissue, a speed of 1668 m/s was used for the degenerated  
15 tissue (Niemenen et al. 2002).

16  
17 The trypsin digestion was stopped by removing the enzyme solution when the front  
18 echoes reached a depth of at least 60% of the total cartilage thickness. The specimens  
19 were immediately washed with physiological saline and stored in a refrigerator until the  
20 histological analysis was performed.

## 1    *Histology*

2    All control and trypsin digested samples were fixed in a 10% buffered formalin and then  
3    quickly decalcified in a 10% EDTA solution, using an ultrasound method reported by  
4    Guo et al. (2005), until the bone tissue could easily be cut with a scalpel. Paraffin  
5    sections, 4 $\mu$ m, were prepared using a rotatory microtome (Lecia RM-2135, Cambrigde,  
6    UK). During section trimming, care was taken to obtain sections proximal to the center  
7    part of the specimen, where the region examined by ultrasound was located. Then, the  
8    deparaffined sections were stained with safranin O (Cat. No. F7258, SiGMA, MO, USA)  
9    and contra-stained with fast green (Cat. No. S-2255, SiGMA, MO, USA). The sections  
10    were examined by an imaging system including a microscope (Model FN-S2N, Nikon,  
11    Japan) and a digital camera (DXM 1200X, Nikon, Japan). In optical micrographs, red  
12    color stained by safranin O indicated the presence of PGs (Leung et al. 1999; Qin et al.  
13    2002). The depth of the trypsin digested zone estimated by measuring the depth of the  
14    fast green-stained zone in the histological image was normalized by the full cartilage  
15    thickness. For each specimen, the digestion fraction was estimated from three histological  
16    sections, averaged and compared to the ultrasound measurement.

17

## 18    **RESULTS**

19    The digestion depth is represented as a function of time in Fig. 3a for all tested specimens.  
20    The average digestion depths at 1 hr, 2 hr, and 3 hr were  $0.76\pm0.10$  mm,  $1.02\pm0.12$  mm,  
21    and  $1.23\pm0.14$  mm, respectively. Fig. 3b shows the relationship between the digestion  
22    depth and the required trypsin treatment time. The error bars are the standard deviations  
23    over the 10 specimens. A 3<sup>rd</sup> order polynomial function was used to fit this relationship

1 ( $R^2 = 0.9999$ ). For a cartilage specimen with a given thickness, the approximate digestion  
2 time can be calculated from this relationship.

3  
4 A comparison of ultrasound data and histological sections in terms of digestion depth is  
5 shown in Fig. 4 for two typical specimens. Fig. 4a, 4b and 4c represent respectively the  
6 histological section of a specimen of undigested cartilage (control sample), the M-mode  
7 data showing the complete digestion process from the cartilage surface to the bone, and  
8 the histological section of the completely digested sample (specimen 8). Fig. 4d, 4e and  
9 4f represent the same types of images for an incompletely digested specimen (specimen  
10 1). The results of ultrasound and histological measurements of the digestion fraction are  
11 shown in Fig. 5. With ultrasound, the final digestion fraction ranged from 64% to 99% of  
12 the sample full-thickness. A correlation was found between the two types of  
13 measurement ( $R^2 = 0.63$ ,  $p < 0.05$ ), although a significant bias (0.64) was found between  
14 the ultrasound and histological measurements. For 7 out of 10 specimens, the digestion  
15 fraction measured by histological sections was larger than that measured with ultrasound.  
16 Also, it was found that ultrasound measurements correlated better with histology for  
17 completely digested samples than for samples that were only partially digested. The  
18 potential reasons are discussed in the next section. Therefore, the cartilage full-thickness  
19 measured by ultrasound was correlated with both histological and digital caliper  
20 measurements for both normal cartilage and digested cartilage (slope  $\approx 1$ ,  $R^2 \approx 0.9$ ) (Fig.  
21 6). A statistical analysis (paired-samples t-test) of the full-cartilage thickness obtained  
22 using any of the three measurement methods, showed that there was no significant

1 difference between digested and undigested samples ( $p > 0.9$ ). The average full-thickness  
2 of the control samples measured by ultrasound, digital caliper and histology was  
3  $1.76 \pm 0.46$  mm,  $1.74 \pm 0.41$  mm, and  $1.82 \pm 0.47$  mm, respectively; that of the digested  
4 samples was  $1.78 \pm 0.48$  mm,  $1.72 \pm 0.44$  mm, and  $1.82 \pm 0.42$  mm, respectively.

5  
6 The transient speed of the digestion front echo was calculated at different time points for  
7 the first three hours. The averaged transient speed over all samples is shown as a function  
8 of time in Fig. 7a. Fig. 7b shows the digestion front speed as a function of depth in the  
9 tissue. It can be seen from Fig. 7 that the digestion speed decreased with increasing tissue  
10 depth. The digestion speed was found to be faster in the superficial layer of the cartilage  
11 samples ( $0.61 \pm 0.16$   $\mu\text{m/s}$ , mean  $\pm$  SD) than in deeper layers ( $0.04 \pm 0.02$   $\mu\text{m/s}$  at 70%  
12 of the full thickness).

## 13 14 **DISCUSSION**

15 A relatively good correlation was found between ultrasound and histology in the  
16 measurements of the digestion fraction ( $R^2 = 0.63$ ,  $p < 0.05$ ). However, for partially  
17 digested samples, the digestion fraction measured in histology was higher than that  
18 estimated using ultrasound. This difference could potentially be explained by a number of  
19 factors affecting these two techniques. On the histology side, these factors might include  
20 tissue shrinkage due to the fixation process, limitation in the staining by safranin O, and a  
21 potential residual digestion by trypsin between the end of the ultrasound experiments and  
22 the histological process. On the ultrasound side, the only factor is a potential difference in  
23 the speed of sound between digested and undigested tissues.

1  
2 Although, tissue shrinkages or deformations due to fixation processes have been reported  
3 in literature, the effects of the fixation by formalin, which has been used in our study, are  
4 minimal (Luna 1992). In this study we made the assumption that if shrinkage occurs,  
5 digested and undigested tissues will be affected in the same proportion. This hypothesis  
6 seemed to be verified in our experiments, since no significant difference in total thickness  
7 was found between partially digested samples and their controls. Therefore, shrinkage  
8 should not affect the digestion fraction, which represents the depth of PGs digestion  
9 normalized by the total tissue thickness.

10  
11 Staining by safranin O, on the other hand, might affect our histological findings. Indeed,  
12 a study published by Camplejohn and Allard (1988) showed that some PGs (chondroitin  
13 sulphate and keratan sulphate) were still present in regions of the cartilage not stained by  
14 safranin O. Therefore, this would lead, in our experiments, to an overestimation of the  
15 depth of digestion, since it was estimated by measuring the depth of the region unstained  
16 by safranin O. Consequently, the digestion fraction would be overestimated.

17  
18 Some residual digestion by trypsin might have occurred as well between the time the  
19 trypsin solution was removed from the bath and the time the tissues were fixed for  
20 histology. In future experiments, this could be prevented by using enzyme inhibitors to  
21 stop the digestion by trypsin (Nieminen et al. 2002; Qin et al. 2002). This would require  
22 investigating the dynamic of the inhibition process, which could be potentially done  
23 using our ultrasound technique.

1  
2 Difference in the speed of sound between digested and undigested tissues might affect  
3 digestion fraction measured in ultrasound. Previous studies have reported that the  
4 ultrasound speed in PG-depleted cartilages is lower than in normal tissues (Joiner et al.  
5 2001; Nieminen et al. 2002; Toyras et al. 1999). However, if we assume a constant speed  
6 of sound both in digested and undigested tissues in our experiments, the thickness of PG-  
7 depleted specimens would be overestimated. Furthermore, no significant difference was  
8 found in cartilage thickness between the PG-depleted specimens and their respective  
9 control using caliper, ultrasound and histology. Since a good correlation was found in the  
10 measurement of the total cartilage thickness between histology and ultrasound, we can  
11 also conclude that the choice of a speed sound of 1668 for the digested samples was  
12 probably accurate. From this analysis, we can infer that the difference in digestion  
13 fraction between histology and ultrasound is probably due to an inaccurate estimation of  
14 the digestion depth of histology.

15  
16 The speed of digestion was found to decrease as increasing of tissue depth. This tendency  
17 is related to the distribution of the PG content, which has been reported to increase as a  
18 function of the tissue depth in normal articular cartilage (Mow and Guo, 2002; Wang et  
19 al., 2002). This implies that more trypsin is needed to digest the PGs deep in the tissue  
20 than at its superficial zone. This could slow down the trypsin penetration and thus the  
21 digestion process in the deeper region of the tissue. These results are consistent with  
22 results obtained by Moody et al. (2006), who showed that, for a given time of exposure  
23 and a given concentration of trypsin, the dynamic of PGs digested by this agent depends  
24 on the concentration of PGs at different depths in the tissue. In addition, this study

1 provides evidence of the variations in digestion by trypsin between different samples, as  
2 it is also reported in Moody's study. As shown in Fig. 3, sample 1 and sample 8, which  
3 are of equivalent thickness, behaved differently under exposure to trypsin. The dynamic  
4 of the diffusion of trypsin from the surface to the deepest region in the cartilage definitely  
5 requires further investigations.

6  
7 In summary, our experiments demonstrated the feasibility of monitoring the digestion of  
8 PGs in real-time using an ultrasonic technique. Our results suggest that this technique  
9 might be better suited than histology to estimate the depth of digestion by trypsin for two  
10 reasons. First, this technique can evaluate the dynamic of the digestion in real-time.  
11 Secondly, the echo reflected at the interface between digested and undigested tissue  
12 represents a real marker of a change in local mechanical properties of the tissue, which  
13 are linked to the content in PGs in the tissue. Our results also provide information about  
14 the progressive depletion of PGs from the cartilage induced by trypsin. It was found that  
15 the digestion depth could be described as a 3<sup>rd</sup> order polynomial function of the exposure  
16 time to trypsin. This ultrasound method could be used for other *in-vitro* models of OA  
17 based on PG degeneration.

## 18 19 **Acknowledgements**

20 This project was partially supported by the Research Grant Council of Hong Kong  
21 (PolyU5199/02E, PolyU 5245/03E) and The Hong Kong Polytechnic University.

## References

- Adam C, Eckstein F, Milz S, and Putz R. The distribution of cartilage thickness within the joints of the lower limb of elderly individuals. *J Anatomy* 1998; 193: 203-214.
- Adler RS, Dedrick DK, Laing TJ, Chiang EH, Meyer CR, Bland PH, Rubin JM. Quantitative assessment of cartilage surface roughness in osteoarthritis using high frequency ultrasound. *Ultrasound Med Biol*. 1992; 18(1): 51-58.
- Agemura DH, O'Brien WD, Olerud JE, Chun LE, and Eyre DE. Ultrasonic propagation properties of articular cartilage at 100 MHz. *J Acoust Soc Am* 1990; 87: 1786-1791.
- Armstrong CG, Mow VC. Variations in the intrinsic mechanical properties of human cartilage with age, degeneration and water content. *J Bone Joint Surg* 1982; 64A: 88-94.
- Batiste DL, Kirkley A, Laverty S, Thain LM, Spouge AR, Holdsworth DW. Ex vivo characterization of articular cartilage and bone lesions in a rabbit ACL transection model of osteoarthritis using MRI and micro-CT. *Osteoarthritis Cartilage* 2004; 12(12): 986-996.
- Camplejohn KL, Allard SA. Limitations of safranin 'O' staining in proteoglycan-depleted cartilage demonstrated with monoclonal antibodies. *Histochemistry*. 1988; 89(2):185-188.
- Cherin E, Saied A, Laugier P, Netter P, and Berger G. Evaluation of acoustical parameter sensitivity to age-related and osteoarthritic changes in articular cartilage using 50 MHz ultrasound. *Ultrasound Med Biol* 1998; 24: 341-354.
- Cherin E, Saied A, Pellaumail B, et al. Assessment of rat articular cartilage maturation using 50-MHz quantitative ultrasonography. *Osteoarthritis Cartilage* 2001; 9: 178-186.
- Flahiff CM, Kraus VB, Huebner JL, Setton LA. Cartilage mechanics in the guinea pig model of osteoarthritis studied with an osmotic loading method. *Osteoarthritis Cartilage* 2004; 12: 383-388.
- Fortin M, Buschmann MD, Bertrand MJ, Foster FS, and Ophir J. Dynamic measurement of internal solid displacement in articular cartilage using ultrasound backscatter. *J Biomech* 2003; 36: 443-447.
- Guo X, Lam WL, Zheng YP. Rapid and quantified decalcification of bone: apparatus and methods. No. 10/510,450. Oct 2005 (PolyU IP174A). US Patent pending.
- Hattori K, Mori K, Habata T, Takakura Y, Ikeuchi K. Measurement of the mechanical condition of articular cartilage with an ultrasonic probe: quantitative evaluation using wavelet transformation. *Clinic Biomech* 2003; 18: 553-557.
- Hattori K, Takakura Y, Ishimura M, Tanaka Y, Habata T, Ikeuchi K. Differential acoustic properties of early cartilage lesions in living human knee and ankle joints. *Arthritis Rheum* 2005; 52(10): 3125-3131.
- Joiner GA, Bogoch ER, Pritzker KP, Buschmann MD, Chevrier A, and Foster FS. High frequency acoustic parameters of human and bovine articular cartilage following experimentally-induced matrix degradation. *Ultrasonic Imaging* 2001; 23: 106-116.



1 Jurvelin JS, Rasanen T, Kolmonen P, and Lyyra T. Comparison of optical, needle probe  
2 and ultrasonic techniques for measurement of articular cartilage thickness. J  
3 Biomechanics 1995; 28: 231-235.

4 Kim HKW, Babyn PS, Harasiewicz KA, Gahunia HK, Pritzker FPH, and Foster FS.  
5 Imaging of immature articular cartilage using ultrasound backscatter microscopy at 50  
6 MHz. J Orthop Res 1995; 13: 963-970.

7 Laasanen MS, Toyras J, Hirvonen J, Saarakkala S, Korhonen RK, Nieminen MT,  
8 Kiviranta I, Jurvilin JS. Novel mechano-acoustic technique and instrument for  
9 diagnosis of cartilage degeneration. Physiol Meas 2002; 23: 491-503.

10 Lai WM, Hou JS, Mow VC. A triphasic theory for the swelling and deformation  
11 behaviors of articular cartilage. J Biomech Eng 1991; 113: 245-258.

12 Lefebvre F, Graillat N, Chérin E, Berger G, and Saïed A, Automatic three  
13 dimensional reconstruction and characterization of articular cartilage from high  
14 resolution ultrasound acquisition. Ultrasound Med Biol 1998; 24: 1369-1381.

15 Leung KS, Qin L, Leung MCT, Fu LLK, Chan CW. Decrease in proteoglycans content of  
16 the remaining patellar articular cartilage after partial patellectomy in rabbits. J Clin  
17 Exp Rheumatol 1999; 17: 597-600.

18 Luna LG. Histopathologic methods and color atlas of special stains and tissue artifacts.  
19 Gaithersburg, MD: American Histolabs, Inc., 1992. pp. 22-23.

20 Lyons TJ, McClure SF, Stoddart RW, and McClure J. The normal human chondro-  
21 osseous junctional region: evidence for contact of uncalcified cartilage with  
22 subchondral bone and marrow spaces. Musculoskeletal Disorders 2006; 7: 52-60.

23 Maroudas A. Balance between swelling pressure and collagen tension in normal and  
24 degenerate cartilage. Nature 1976; 260: 808-809.

25 Martini FH. Fundamentals of anatomy and physiology (6<sup>th</sup> Edition), Upper Saddle River,  
26 NJ: Prentice Hall, 2004.

27 Moody HR, Brown CP, Bowden JC, Crawford RW, McElwain DL, Oloyede AO. In vitro  
28 degradation of articular cartilage: does trypsin treatment produce consistent results? J  
29 Anat. 2006; 209(2): 259-267.

30 Mow VC, Gu WY, Chen FH. Structure and function of articular cartilage and meniscus.  
31 In: Mow VC, Huiskes R, ed. Basic Orthopaedic Biomechanics and Mechano-Biology  
32 (3<sup>rd</sup> Edition). Lippincott Williams & Wilkins, PA, USA. 2005. pp. 181-258.

33 Mow VC, Guo XE. Mechano-electrochemical properties of articular cartilage: their  
34 inhomogeneities and anisotropies. Annu Rev Biomed Eng 2002; 4: 175-209.

35 Myers SL, Dines K, Brandt DA, Brandt KD, and Alvrecht ME. Experimental assessment  
36 by high frequency ultrasound of articular cartilage thickness and osteoarthritic changes.  
37 J Rheumatology 1995; 22: 109-116.

38 Narmoneva DA, Wang JY, Setton LA. Nonuniform swelling-induced residual strains in  
39 articular cartilage. J Biomech 1999; 32: 401-408.

- 1 Narmoneva DA, Cheung HS, Wang JY, Howell DS, Setton LA. Altered swelling  
2 behavior of femoral cartilage following joint immobilization in a canine model. *J*  
3 *Orthop Res* 2002; 20: 83-91.
- 4 Nieminen HJ, Toyras J, Rieppo J, Nieminen MT, Hirvonen J, Korhonen R, Jurvelin JS.  
5 Real-time ultrasound analysis of articular cartilage degradation in vitro. *Ultrasound*  
6 *Med Biol* 2002; 28(4): 519-525.
- 7 Patil SG, Zheng YP, Wu JY, Shi J. Measurement of depth-dependency and anisotropy of  
8 ultrasound speed of bovine articular cartilage in vitro. *Ultrasound Med Biol* 2004;  
9 30(7): 953-963.
- 10 Pellaumail B, Watrin A, Loeuille D, Netter P, Berger G, Laugier P, Saied A. Effect of  
11 articular cartilage proteoglycan depletion on high frequency ultrasound backscatter.  
12 *Osteoarthritis Cartilage*. 2002; 10(7): 535-541.
- 13 Qin L, Zheng Y, Leung C, Mak A, Choy W, Chan K. Ultrasound detection of trypsin-  
14 treated articular cartilage: its association with cartilaginous proteoglycans assessed by  
15 histological and biochemical methods. *J Bone Miner Metab* 2002; 20(5): 281-287.
- 16 Raynauld JP, Martel-Pelletier J, Berthiaume MJ, Beaudoin G, Choquette D, Haraoui B,  
17 Tannenbaum H, Meyer JM, Beary JF, Cline GA, Pelletier JP. Long term evaluation of  
18 disease progression through the quantitative magnetic resonance imaging of  
19 symptomatic knee osteoarthritis patients: correlation with clinical symptoms and  
20 radiographic changes. *Arthritis Res Ther* 2006; 8(1): R21
- 21 Saarakkala S, Laasanen MS, Jurvelin JS, Torronen K, Lammi MJ, Lappalainen R, Toyras  
22 J. Ultrasound indentation of normal and spontaneously degenerated bovine articular  
23 cartilage. *Osteoarthritis Cartilage* 2003; 11: 697-705.
- 24 Saied A, Cherin E, Gaucher H, et al. Assessment of articular cartilage and subchondral  
25 bone: subtle and progressive changes in experimental osteoarthritis using 50 MHz  
26 echography in vitro. *J Bone Mineral Res* 1997; 12: 1378-1387.
- 27 Sandy JD. Proteolytic degradation of normal and osteoarthritic cartilage matrix. In:  
28 Brandt KD, Doherty M, Lohmander LS, ed. *Osteoarthritis*, Oxford; New York: Oxford  
29 University Press, 2003. pp. 82-92.
- 30 Senzig DA, Forster FK, and Olerud JE. Ultrasonic attenuation in articular cartilage. *J*  
31 *Acoust Soc of Am* 1992; 92: 676-681.
- 32 Torzilli PA, Askari E, Jenkins JT. Water content and solute diffusion properties in  
33 articular cartilage. In: Mow VC, Ratcliffe A, Woo SLY, ed. *Biomechanics of*  
34 *diarthrodial joints (Vol. I)*, Springer-Verlag, New York Inc., 1990. pp. 363-390.
- 35 Toyras J, Rieppo J, Nieminen MT, Helminen HJ, Jurvelin JS. Characterization of  
36 enzymatically induced degradation of articular cartilage using high frequency  
37 ultrasound. *Phys Med Biol* 1999; 44: 2723-2733.
- 38 Toyras J, Lyyra-Laitinen T, Niinimäki M, Lindgren R, Nieminen MT, Kiviranta I,  
39 Jurvelin JS. Estimation of the Young's modulus of articular cartilage using an  
40 arthroscopic indentation instrument and ultrasonic measurement of tissue thickness. *J*  
41 *Biomechanics* 2001; 34 (2): 251-256.

- 1 Wang CC, Guo XE, Sun DN, Mow VC, Ateshian GA, Hung CT. The functional  
2 environment of chondrocytes within cartilage subjected to compressive loading: A  
3 theoretical and experimental approach. *Biorheology*. 2002; 39(1-2): 11-25.
- 4 Wang Q, Zheng YP. Non-contact evaluation of osmosis-induced shrinkage and swelling  
5 behavior of articular cartilage in situ using high-frequency ultrasound. *Instrument Sci*  
6 *Technol* 2006; 34(3): 317-334.
- 7 Wang Q, Zheng YP, Niu HJ, Mak AFT. Extraction of mechanical properties of articular  
8 cartilage from osmotic swelling behavior monitored using high frequency ultrasound.  
9 *ASME Transactions J Biomech Eng* 2007; 129: 413-422.
- 10 Yang CP, Lee CL, Chen TW, Lee S, Weng MC, Huang MH. Ultrasonographic findings  
11 in hemiplegic knees of stroke patients. *Kaohsiung J Med Sci* 2005; 21: 70-77.
- 12 Yao JQ and Seedhom BB. Ultrasonic measurement of the thickness of human articular  
13 cartilage in situ. *Rheumatology* 1999; 38: 1269-1271.
- 14 Zheng YP, Mak AFT. An Ultrasound indentation system for biomechanical properties  
15 assessment of soft tissues in-vivo. *IEEE Trans Biomed Eng* 1996; 43: 912-918.
- 16 Zheng YP, Ding CX, Bai J, Mak AFT, Qin L. Measurement of the layered compressive  
17 properties of trypsin-treated articular cartilage: an ultrasound investigation. *Med Biol*  
18 *Eng Comput* 2001; 39: 534-541.
- 19 Zheng YP, Mak AFT, Lau KP, and Qin L. Ultrasonic measurement for in-vitro depth-  
20 dependent equilibrium strains of articular cartilage in compression. *Phys Med Biol*  
21 2002; 47: 3165-3180.
- 22 Zheng YP, Bridal SL, Shi J, Saied A, Lu MH, Jaffre B, Mak AFT, Laugier P. High  
23 resolution ultrasound elastomicroscopy imaging of soft tissues: System development  
24 and feasibility. *Phys Med Biol*. 2004a; 49: 3925-3938.
- 25 Zheng YP, Shi J, Qin L, Patil SG, Mow VC, Zhou KY. Dynamic depth-dependent  
26 osmotic swelling and solute diffusion in articular cartilage monitored using real-time  
27 ultrasound. *Ultrasound Med Biol* 2004b; 30: 841-849.
- 28 Zheng YP, Niu HJ, Mak AFT, and Huang YP. Ultrasonic Measurement of depth-  
29 dependent transient behaviors of articular cartilage under compression. *J*  
30 *Biomechanics* 2005; 38:1830-1837.
- 31 Zhu W, Mow VC, Koob TJ, Eyre DR. Viscoelastic shear properties of articular cartilage  
32 and the effects of glycosidase treatments, *J Orthop Res* 1993; 11(6): 771-781.

33

## Figure Captions

Fig. 1 (a) The cartilage-bone plug was cut into two parts (1/3 and 2/3). (b) Schematic of the ultrasound experimental setup. Samples were fixed at the bottom of the container filled with saline or trypsin solution.

Fig. 2 Typical M-mode image showing the progression of the digestion induced by trypsin. Markers along the digestion front are indicating some of the positions of the front used for the calculation of the interpolation. RF ultrasound echoes (a, b and c) were extracted from the M-mode image. The echoes from the digestion front, which are circled in the RF signals, are pointed by black arrows in M-mode image.

Fig. 3 (a) The transient digestion depth as a function of time for the 10 specimens. (b) Nonlinear relationship between the digestion depth and the digestion time.

Fig. 4 Comparison of M-mode images with histological sections for a completely digested cartilage (a,b,c) and an incompletely digested cartilage (d,e,f). (a) and (d) are histological sections of the control undigested samples; (b) and (e) are M-mode images showing the digestion front dynamic; (c) and (f) are histological sections from the digested samples. Black triangle indicates the cartilage surface. Dashed line in (c, f) indicates the interface between safranin O and fast green stained regions. The scale is 200  $\mu\text{m}$ .

1 Fig. 5 Correlation between the digestion fractions measured using histology and  
2 ultrasound.

3


4 Fig. 6 Correlation of cartilage full-thickness measured by: (a) digital caliper versus  
5 ultrasound; (b) histology versus ultrasound.

6


7 Fig. 7 (a) Averaged digestion speed as a function of time. (b) Averaged digestion speed  
8 as a function of depth. Error bars represent the standard deviations over 10 specimens.

9

10

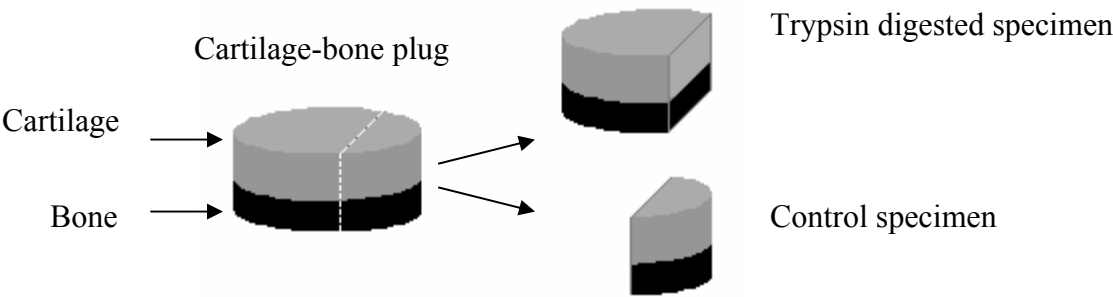

(a)

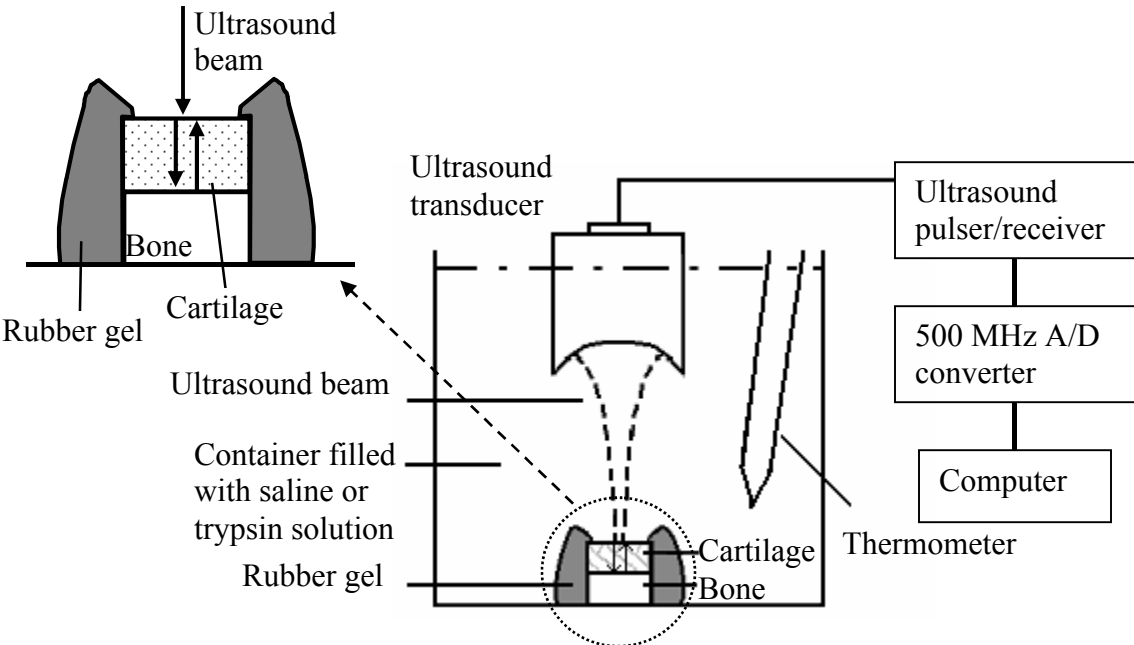

(b)

Fig. 1

Figure 2  
[Click here to download Figure: Fig2.doc](#)



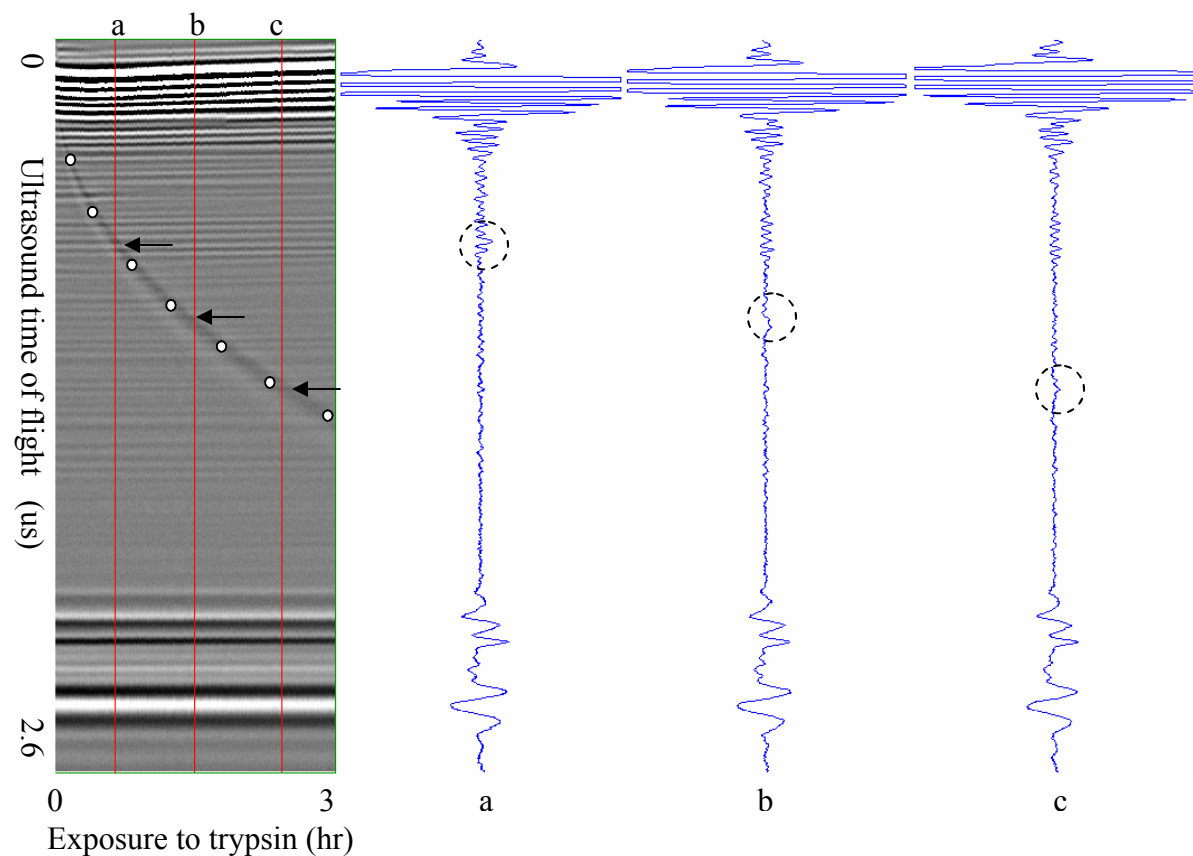


Fig. 2

Figure 3  
[Click here to download Figure: Fig3.doc](#)

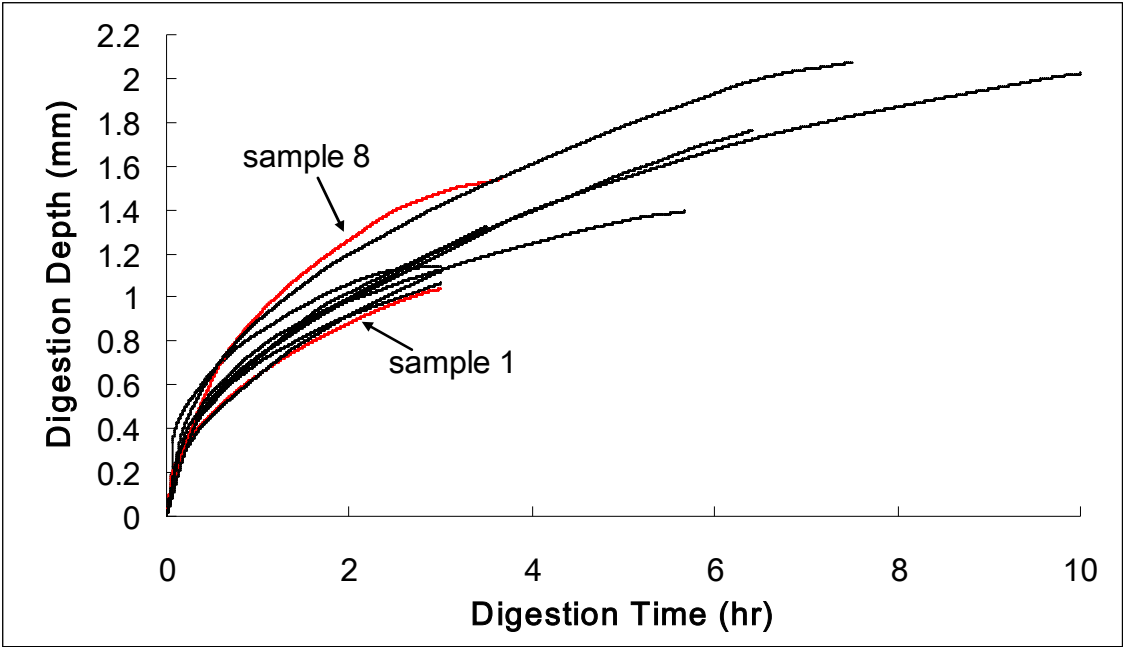

(a)

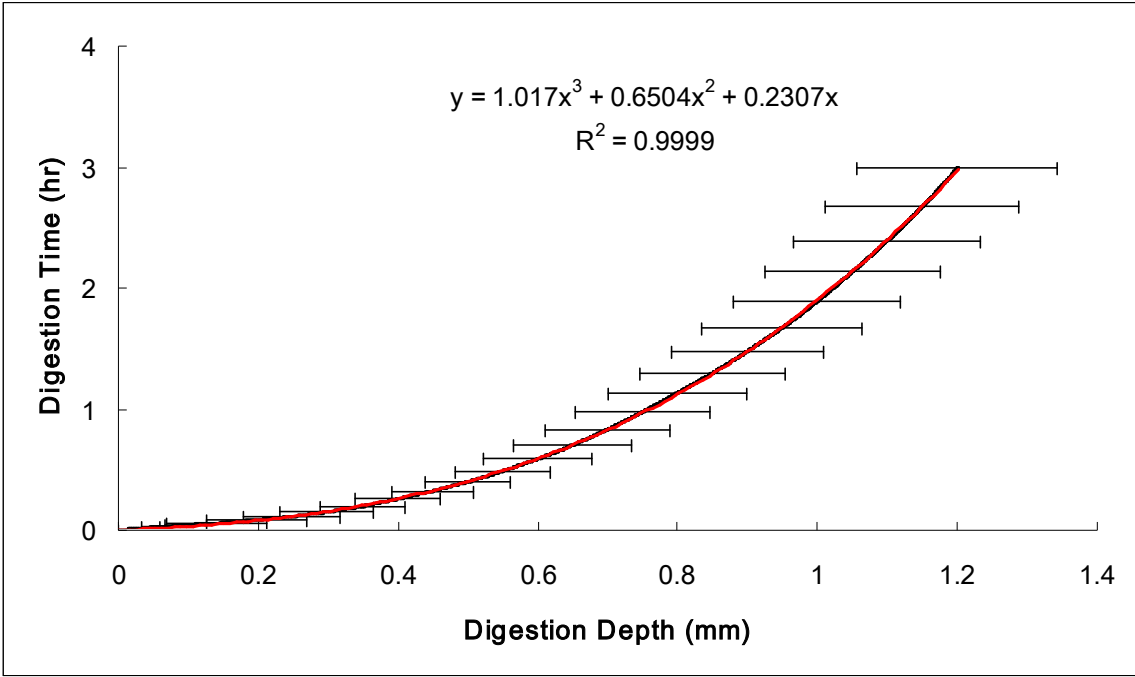

(b)

Fig. 3



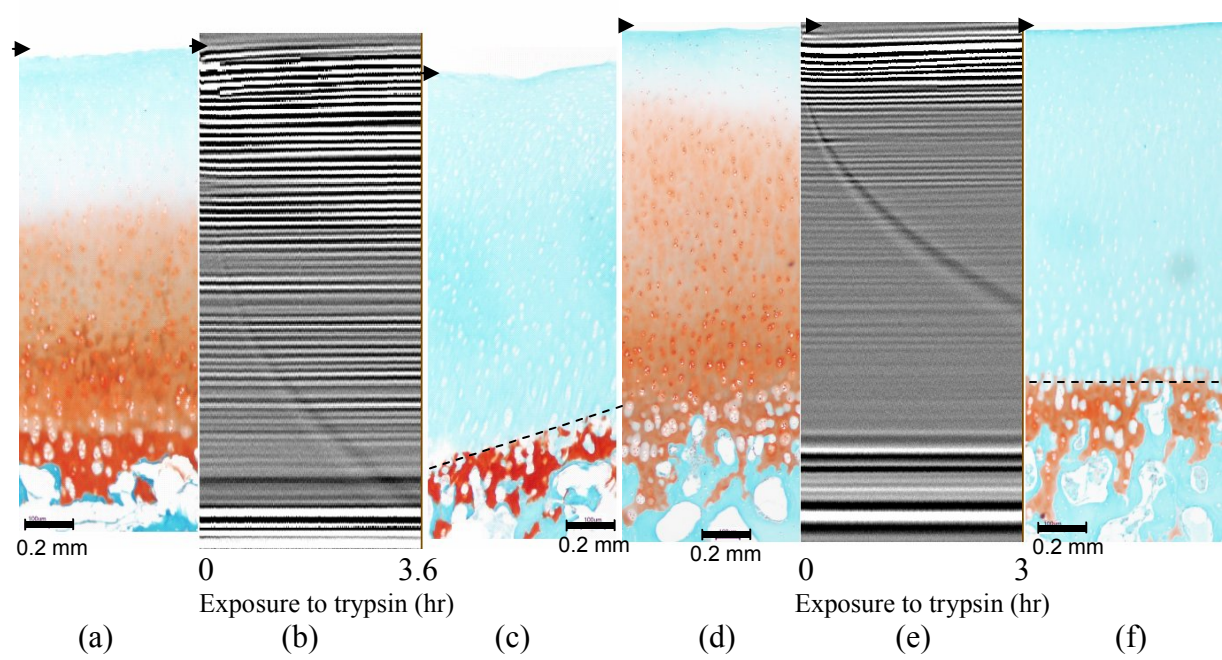


Fig. 4



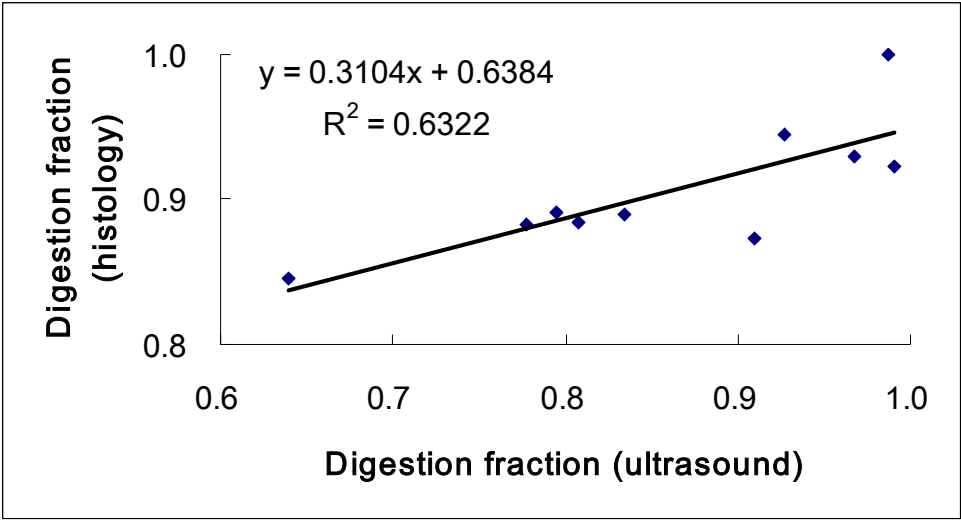


Fig. 5

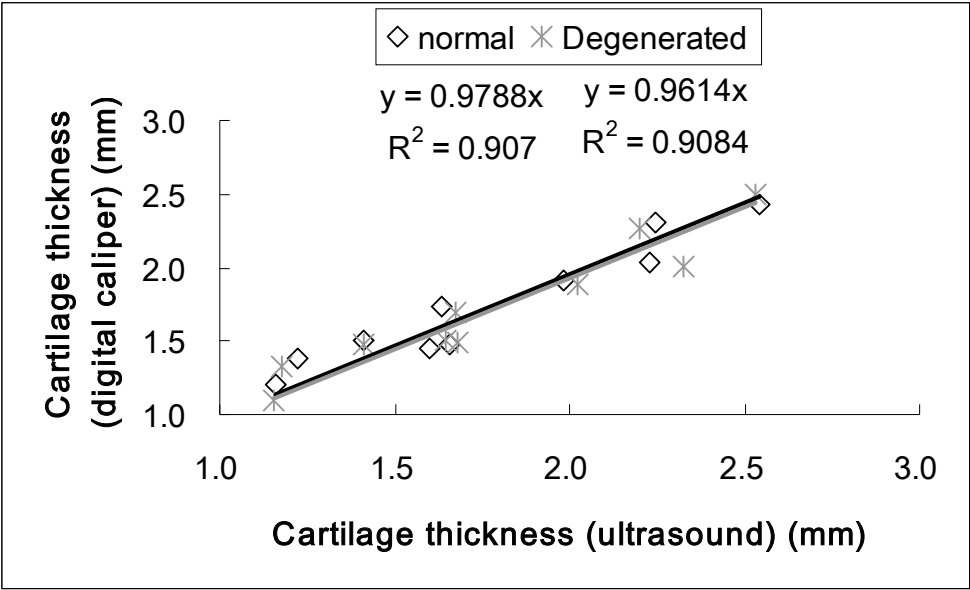


(a)

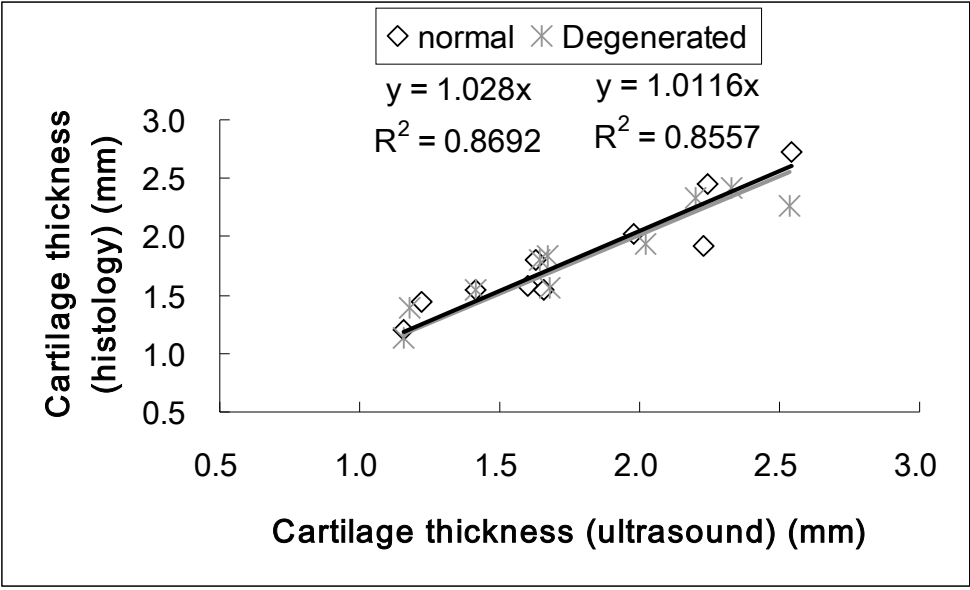


(b)

Fig. 6

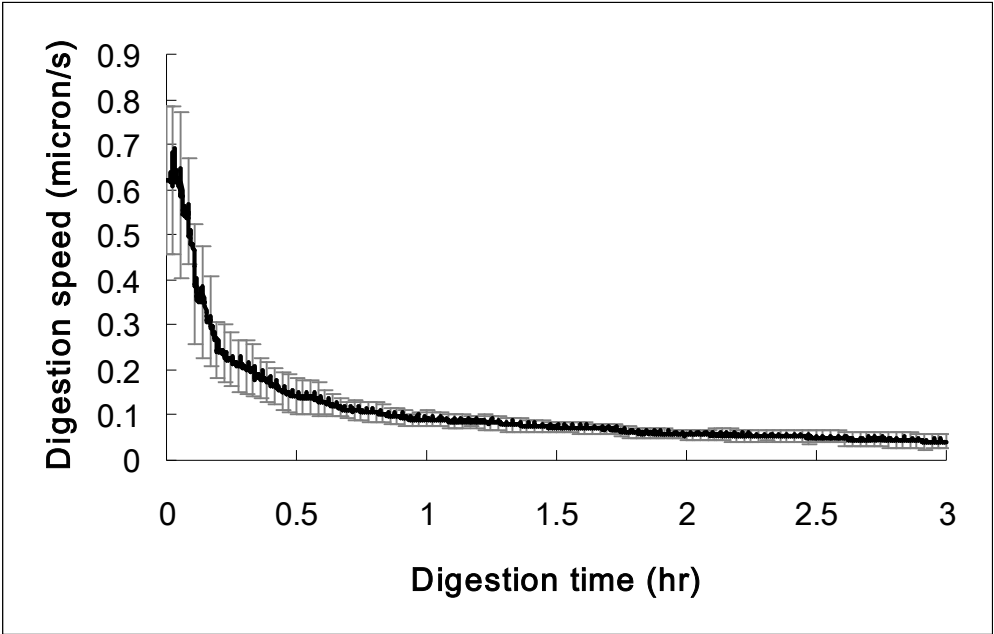

(a)

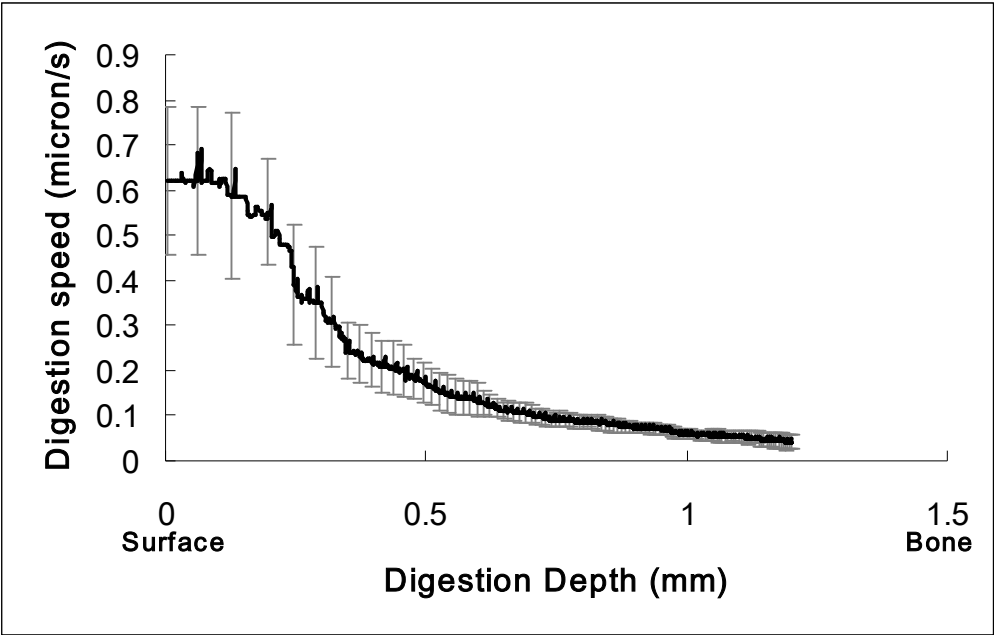

(b)

Fig. 7